

InertSustain[®] Cyano Technical Data

October, 2017



InertSustain Cyano Physical Properties

Silica	: ES Silica Gel
Particle Size	: 3 μm , 5 μm
Surface Area	: 350 m^2/g
Pore Size	: 100 \AA (10 nm)
Bonded Phase	: Cyanopropyl Groups
End-capping	: Yes
Carbon Loading	: 8 %
pH Range	: 2~7.5
USP Code	: L10

Features of InertSustain Cyano

Cyano Column?




- Different selectivity compared to C18 and Phenyl phases. The retention is weaker than a Phenyl phase.
(slide 4~14)

Comparison to Other Cyano Columns

- Workable in both reversed and normal-phase modes.
(slide 15~17)
- Rigorous end-capped treatment provide better peak shapes
(slide 18~19)
- Simply better reproducibility (slide 20)







Comparison between C18 and Phenyl phases (β Blockers)

The separation pattern between Alprenolol and Propranolol were different. Propranolol consist a naphthalene ring which was retained stronger on cyano and phenyl phases due to the pi electron interaction. As a result, the elution pattern was different to a C18 phase.

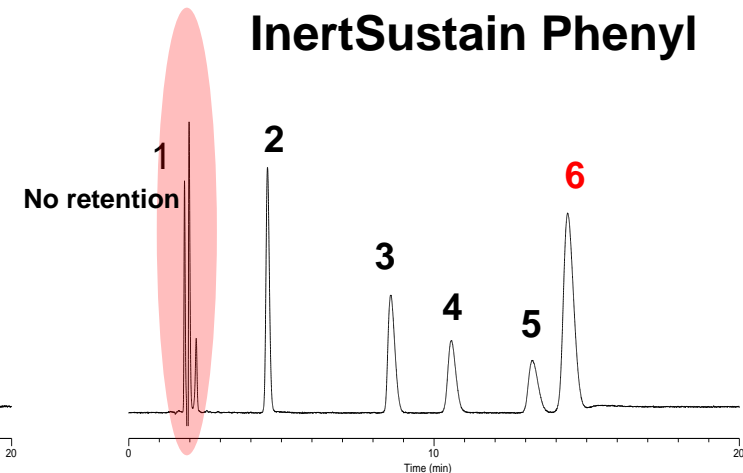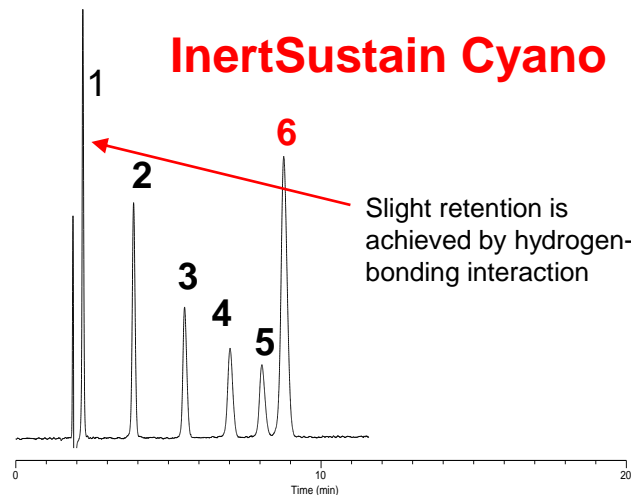

Conditions


Eluent : A) 0.1 % HCOOH B) CH₃CN
 A/B= 80/20,v/v
 Flow Rate : 1.0 mL/min
 Col. Temp. : 40 °C
 Detection : UV 220 nm
 Sample : 1. Atenolol
 2. Acebutolol
 3. Oxprenolol
 4. Labetalol
 5. Alprenolol
 6. Propranolol




Comparison between C18 and Phenyl phases (Strong Bases)

As shown below, inertness to strong basic compounds were confirmed to be satisfactory. The elution pattern is different on a Cyano phase due to the difference in interaction. The interaction on a Cyano phase is mainly pi electron interaction.


InertSustain Cyano



InertSustain C18




InertSustain Phenyl




Conditions

Eluent : A) 5 mM HCOONH₄ B) CH₃CN
A/B = 60/40, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 230 nm
Sample : 1. Uracil
2. Dextromethorphan
3. Berberine




2. Berberine






3. Dextromethorphan

Selectivity ① (Planar Molecule Recognition)



60 % Methanol

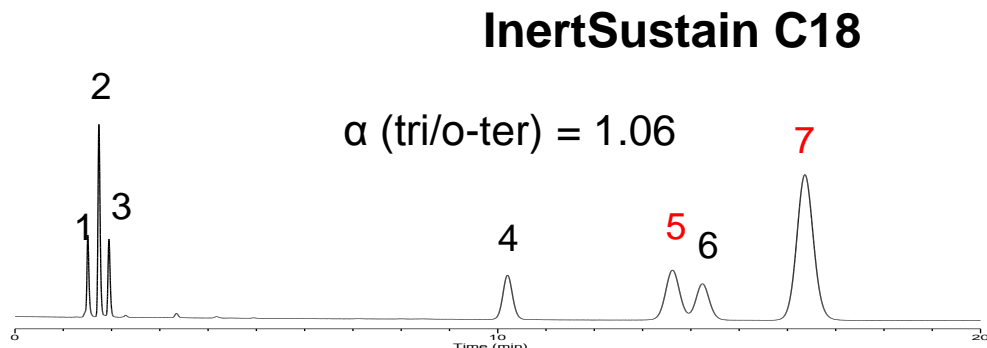

The retention of hydrophobic analytes are weaker on InertSustain Cyano when comparing to Phenyl phases. Analytes consisting benzene rings tend to be retained stronger due to the pi-pi interaction.

Conditions

Eluent : A) CH₃OH B) H₂O

A/B = 80/20, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 254 nm

Sample:

1. Uracil
2. Caffeine
3. Phenol
4. Butylbenzene
5. o-Terphenyl
6. Amylbenzene
7. Triphenylene




5. o-Terphenyl




7. Triphenylene

Selectivity ② (Cis-, Trans-)


InertSustain Cyano

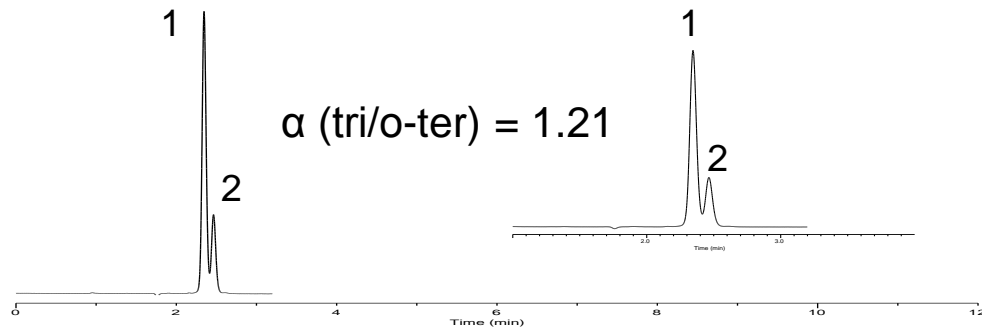

60 % Methanol




InertSustain Phenyl




The separation of cis-, trans- were satisfactory under the following analytical conditions. However, the separation was improved further by decreasing the methanol content.

Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 80/20, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 210nm
Sample : 1. cis-Stilbene
2. trans-Stilbene




InertSustain C18




Selectivity ③ (Ortho-, Meta-)


InertSustain Cyano



60 % Methanol




InertSustain Phenyl




The separation of *o*-, *m*- were satisfactory under the following analytical conditions. However, the separation was improved further by decreasing the methanol content.

InertSustain C18






Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 80/20, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 254 nm
Sample : 1. *o*-Terphenyl
2. *m*-Terphenyl




Hydrogen-Bonding, Electron Withdrawing ①

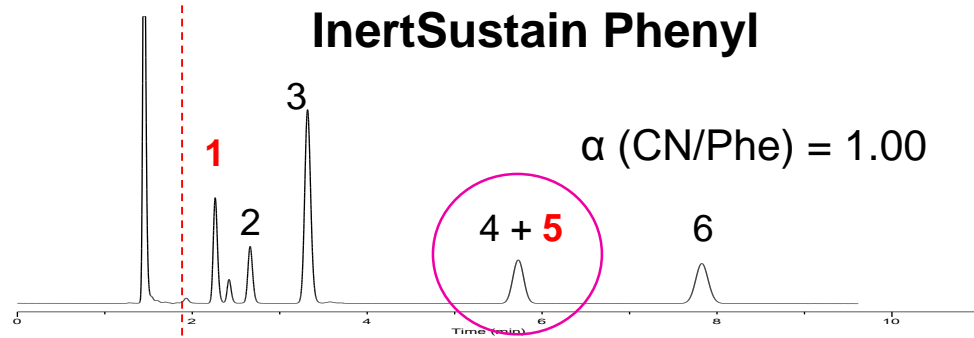


The retention of hydrophobic analytes will be low on InertSustain Cyano when comparing to a C18 phase, however, there is a retention for polar analytes.

Conditions


- Eluent : A) CH₃CN B) 0.1% H₃PO₄
A/B = 25/75, v/v
- Flow Rate : 1.0 mL/min
- Col. Temp. : 40 °C
- Detection : UV 280 nm
- Sample : 1. 4-Hydroxybenzamide
2. Hydroquinone
3. 4-Hydroxybenzoic acid
4. Phenol
5. 4-Hydroxybenzonitril
6. *p*-Nitrophenol



4-Hydroxybenzamide




Phenol




4-Hydroxybenzonitril

Electron Withdrawing ②


InertSustain Cyano



InertSustain Phenyl



InertSustain C18



InertSustain Cyano retains samples consisting high electron withdrawing groups such as nitro groups much efficiently than Phenyl bonded phases.

Conditions


Eluent : A) 0.1 % H_3PO_4
B) CH_3CN
A/B = 75/25, v/v

Flow Rate : 1.0 mL/min


Col. Temp. : 40 °C

Detection : UV 280 nm

Sample : 1. 3,4-Dihydroxy Benzoic Acid
2. Hydroquinone
3. Resorcinol
4. Catechol
5. 4-Methyl Catechol
6. 4-Nitrocatechol



5. 4-Methyl Catechol



6. 4-Nitrocatechol

Comparison of Performance

Planar Selectivity


Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 80/20, v/v

Flow Rate : 1.0 mL/min
Col. Temp.: 40 °C
Detection : UV 254 nm

Sample :

1. Uracil
2. Caffeine
3. Phenol
4. Butylbenzene
5. **o-Terphenyl**
6. Amylbenzene
7. **Triphenylene**



Separation of Cis-trans


Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 80/20, v/v

Flow Rate : 1.0 mL/min
Col. Temp.: 40 °C
Detection : UV 210 nm

Sample :

1. **cis-Stilbene**
2. **trans-Stilbene**



Separation of o, m-


Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 80/20, v/v

Flow Rate : 1.0 mL / min
Col. Temp. : 40 °C
Detection : UV 254 nm

Sample :

1. **o-Terphenyl**
2. **m-Terphenyl**



Electron Withdrawing using NO₂


Conditions

Eluent : A) 0.1 % H₃PO₄ B) CH₃CN
A/B = 75/25, v/v

Flow Rate : 1.0 mL/min
Col. Temp.: 40 °C
Detection : UV 280 nm

Sample :

1. 3,4-Dihydroxy Benzoic Acid
2. Hydroquinone
3. Resorcinol
4. Catechol
5. **4-Methyl Catechol**
6. **4-Nitrocatechol**



Electron Withdrawing using CN


Conditions

Eluent : A) CH₃CN B) 0.1% H₃PO₄
A/B = 25/75, v/v

Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 280 nm

Sample :

1. 4-Hydroxybenzamide
2. Hydroquinone
3. 4-Hydroxybenzoic acid
4. **Phenol**
5. **4-Hydroxybenzonitril**
6. *p*-Nitrophenol



Hydrogen-Bonding using Amide


Conditions

Eluent : A) CH₃CN B) 0.1% H₃PO₄
A/B = 25/75, v/v

Flow Rate : 1.0 mL/min
Col. Temp.: 40 °C
Detection : UV 280 nm







Sample :

1. **4-Hydroxybenzamide**
2. Hydroquinone
3. 4-Hydroxybenzoic acid
4. **Phenol**
5. 4-Hydroxybenzonitril
6. *p*-Nitrophenol



Selectivity of InertSustain Series

InertSustain Cyano provide low retention, but with unique selectivity









Horizontal axis : Hydrophobicity (Retention factor of butylbenzene k_B, CH₃OH:H₂O=80:20)
 Vertical axis : Separation factor of each test

C18 : InertSustain C18 C8 : InertSustain C8 Phenyl : InertSustain Phenyl
 Swift C18 : InertSustainSwift C18 Swift C8 : InertSustainSwift C8 Phenylhexyl : InertSustain Phenylhexyl
 AQ-C18 : InertSustain AQ-C18

Selectivity of Cyano and Phenyl phases

InertSustain Cyano offer better selectivity compared to Phenyl phases





Horizontal axis : Hydrophobicity (Retention factor of butylbenzene k, CH₃OH:H₂O=80:20)

Vertical axis : Separation factor of each test

Retention for Polar Analytes


InertSustain Cyano do not offer retention for polar analytes under 100 % aqueous mobile phases



Horizontal axis : Retention factor of Amylbenzene k , $\text{CH}_3\text{OH}:\text{H}_2\text{O}=80:20$
 Vertical axis : Retention factor of neutral, basic and acidic analytes under 100 % aqueous mobile phase

Comparison between Normal and Reversed-Phase Modes


Normal-Phase Mode



Conditions

Eluent : A) Hexane B) Ethanol
A/B = 90/10, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 220 nm


Reversed-Phase Mode




Conditions

Eluent : A) CH₃OH B) H₂O
A/B = 40/60, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 220 nm


Separation may improve in normal-phase mode depending on the sample.




1. Progesterone



2. Corticosterone




3. Prednisone



4. Prednisolone





Analysis of Steroids by Normal-Phase Mode

InertSustain Cyano columns can be used under Normal-Phase mode without any problem.






Conditions

Eluent : A) Hexane B) Ethanol
A/B = 90/10, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 220 nm
Sample : 1. Progesterone
2. Estrone
3. β -Estradiol
4. Corticosterone
5. Hydrocortisone



Inertness to Strong Basic Compounds (Under Acidic Mobile Phase)

InertSustain Cyano columns are rigorously end-capped which provide symmetrical peak shapes for strong basic compounds.



Conditions

Eluent : A) 0.1 % H₃PO₄ B) CH₃CN
A/B = 75/25 , v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 230 nm

Sample :



1. Uracil 2. Dextromethorphan 3. Berberine



2. Dextromethorphan






3. Berberine



Inertness to Strong Basic Compounds (Under Neutral Mobile Phase)

At neutral mobile phases, silanol groups present will act like an acidic moiety and will become ionized - increasing the tailing observed with analytes containing basic functional groups. As proven below, InertSustain Cyano does not show excessive tailing or retention of strong basic analytes.



Conditions

Eluent : A) 50 mM HCOONH₄ B) CH₃CN
A/B = 70/30 , v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 230 nm

Sample :



1. Uracil 2. Dextromethorphan 3. Berberine



2. Dextromethorphan








3. Berberine



Chelating Compound

Hinokitiol is a strong chelating compound, which coordinately binds with the surface of residual trace metal impurities, resulting in severe tailing. As shown below, InertSustain Cyano provide superior peak shape for strong chelating compound.



Conditions


Eluent : A) 0.1 % H₃PO₄ B) CH₃CN
A/B = 75/25, v/v

Flow Rate : 1.0 mL / min

Col. Temp. : 40 °C


Detection : UV 310 nm

Sample : Hinokitiol




Reproducibility of Strong Basic Compounds

InertSustain Cyano



Zorbax SB-CN



Observed a variation of inertness from lot-to-lot

Conditions

Eluent : A) CH₃CN B) 0.1% H₃PO₄
A/B = 25/75, v/v

Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C

Detection : UV 230 nm


Sample : 1. Uracil

2. Dextromethorphan

3. Berberine

Application : *o,m,p*-Methylhippuric Acids

It is hard to separate *m,p* using a conventional C18 column. The InertSustain Cyano provided baseline separation due to its' unique selectivity.



Conditions

Column : InertSustain Cyano, (3 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) CH₃CN B) 0.1 % HCOOH
A/B = 1/99, v/v

Flow Rate : 1.0 mL/min

Col. Temp. : 40 $^{\circ}$ C




Detection : UV 220 nm

Sample:


1. *o*-Methylhippuric Acid

2. *p*-Methylhippuric Acid

3. *m*-Methylhippuric Acid



Application : Steroids by Normal-Phase Mode



As the hydrophobicity of analytes are quite similar, failure in separation may be observed under reversed-phase mode. Separation may be improved by using normal-phase mode.

Conditions

Column : InertSustain Cyano, (3 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) Hexane B) Ethanol

A/B = 95/5, v/v

Flow Rate : 1.0 mL/min

Col. Temp. : 40 $^{\circ}$ C

Detection : UV 220 nm

Sample :

1. Progesterone

2. Estrone


3. β -Estradiol

4. Corticosterone


5. Hydrocortisone

6. Prednisone


7. Prednisolone




Progesterone




Estrone




β -Estradiol




Corticosterone



Hydrocortisone




Prednisone



Prednisolone

Application : Antidepressants



Conditions

Column : InertSustain Cyano(3 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) 10 mM HCOONH₄ (0.1% HCOOH) B) CH₃CN(0.1% HCOOH)
A/B = 70/30, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 $^{\circ}$ C


Detection : UV 230 nm

Sample:


- | | | |
|---------------|-----------------|------------------|
| 1. Mianserine | 2. Imipramine | 3. Amitriptyline |
| 4. Sertraline | 5. Clomipramine | |




Mianserine




Imipramine



Amitriptyline




Sertraline



Clomipramine

Application : First-Generation Antihistamines



Conditions

Column : InertSustain Cyano (3 μ m, 150 \times 4.6 mm I.D.)
Eluent : A) 10 mM HCOONH₄(0.1% HCOOH) B) CH₃CN(0.1% HCOOH)
A/B = 70/30, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 220 nm

Sample:


- | | | |
|-----------------------|-----------------|----------------|
| 1. Chlorpheniramine | 2. Triprolidine | 3. Hydroxyzine |
| 4. Homochlorcyclizine | 5. Clemastine | |




Chlorpheniramine




Triprolidine



Hydroxyzine




Homochlorcyclizine



Clemastine

Application : Second-Generation Antihistamines



Conditions

Column : InertSustain Cyano (3 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) 0.1% H₃PO₄ B) CH₃CN
A/B = 70/30, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 220 nm

Sample:


- | | | |
|---------------|---------------|-----------------|
| 1. Epinastine | 2. Ketotifen | 3. Loratadine |
| 4. Azelastine | 5. Cetirizine | 6. Fexofenadine |




Epinastine




Ketotifen




Loratadine



Azelastine




Cetirizine



Fexofenadine

Application : Phytohormones



Conditions

Column : InertSustain Cyano (5 μm , 150 \times 4.6 mm I.D.)

Eluent : A) 0.1% H_3PO_4 B) CH_3OH

A/B = 90/ 0, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40°C


Detection : UV 210 nm

Sample:


1. *t*-Zeatin 2. Kinetin 3. 6-Benzylaminopurine 4. Gibberellin A3
5. Indole-3-acetic acid 6. *t-t*-Abscisic acid 7. *c-t*-Abscisic acid 8. Jasmonic Acid




t-Zeatin




Kinetin




6-Benzylaminopurine




Gibberellin A3




Indole-3-acetic acid



t-t-Abscisic Acid




c-t-Abscisic Acid



Jasmonic Acid

Application : Citrals (geranial, neral)



Conditions

Column : InertSustain Cyano (5 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) 0.1% H_3PO_4 B) CH_3OH
A/B = 60/40, v/v


Flow Rate : 1.0 mL/min

Col. Temp. : 40 $^\circ\text{C}$


Detection : UV 210 nm

Sample:

1. cis-Citral 2. Trans-Citral




cis-Citral
(Neral)



trans-Citral
(Geranial)

Application : Chlorophenols



Conditions

Column : InertSustain Cyano (5 μ m, 150 \times 4.6 mm I.D.)

Eluent : A) 0.1% H₃PO₄ B) CH₃OH

A/B = 60/40, v/v

Flow Rate : 1.0 mL/min

Col. Temp. : 40 °C


Detection : UV 280 nm

Sample:


1. 2,6-Dichlorophenol
2. 2,4-Dichlorophenol
3. 2,4,5-Trichlorophenol
4. 3,4,5-Trichlorophenol
5. 2,3,4,5-Tetrachlorophenol
6. Pentachlorophenol

Application : Nortriptyline Hydrochloride Capsules

USP Method



Nortriptyline Hydrochloride Capsules



USP Column: 5 μ m, 150 \times 4.6 mm I.D. (L10)

System suitability requirements:

Efficiency (N) : > 500

Tailing factor : < 3.0

Sample Conc. : 0.38 mg/mL (in Methanol)

Mobile Phase : ACN : CH₃OH : 12 mM Potassium phosphate (pH 6.7)
= 40 : 43 : 17


Flow Rate : 2.5 mL

Detection : UV 239 nm


Injection : 5 μ L

Application : Sertraline Hydrochloride

USP Method



Sertraline Hydrochloride



USP Column: 5 μ m, 150 \times 4.6 mm I.D. (L10)

System suitability requirements:

Tailing factor : < 2.0

Sample Conc. : 0.050 mg/mL (in Mobile Phase)

Mobile Phase : CH₃OH : 0.1% (v/v) Phosphate acid
= 1 : 1

Flow Rate : 1.5 mL


Detection : UV 210 nm

Colum Temp. : 30 $^{\circ}$ C


Injection : 10 μ L

Application : Tetracaine Hydrochloride Ophthalmic Solution

USP Method



Tetracaine Hydrochloride Ophthalmic Solution



USP Column: 5 μ m, 150 \times 4.6 mm I.D. (L10)

System suitability requirements:

Efficiency (N) : >500

Tailing factor : < 2.0

Sample Conc. : 0.1 mg/mL (in Water)

Mobile Phase : ACN : 10 mM Ammonium phosphate (pH 3.0)
= 30 : 70

Flow Rate : 2.0 mL

Detection : UV 280 nm

Injection : 10 μ L

GL Sciences' Reversed-Phase HPLC Column Selection Guide

InertSustain C18

- First Choice C18 Column

InertSustain AQ-C18

- Ideal for Maximizing Retention for Highly Polar Compounds in Reversed Phase Methods with Highly Aqueous Mobile Phases

InertSustainSwift C18

- Rapid Elution of Samples in Isocratic Methods and Rapid Column Equilibration Time in Gradient Methods

Inertsil ODS-HL

- Ultra High Retentivity, High-Density Bonding of C18 Phase
- Ideal for Separation of Basic Molecules & its Related Substances, Process Impurities

InertSustain Phenyl

- Provides not only pi-pi interactions, but also hydrogen bonding secondary interactions
- Ideal for critical resolving compounds (e.g. metabolites) that could not be separated on a C18 phase

InertSustain Phenylhexyl

- Deliver complementary selectivity to straight alkyl-chain columns, but with slight pi-pi interactions
- Industry leading inertness, lot-to-lot reproducibility and low back pressure

InertSustain Cyano

- First choice USP L10 column
- The most Reliable and Reproducible Cyano column

GL Sciences' HILIC HPLC Column Selection Guide

InertSustain Amide


- Excellent for those hard to retain compounds using an ODS column
- First choice HILIC column under HILIC Mode Separation

InertSustain NH2

- A Primary Amine Bonded column preventing anomer resolution with easy sugar analysis at low temperature
- Highly reproducible results with exceptional stability and durability that will maintain performance over the lifetime of the method


Explanation of Analytical Tests and Conditions

Selectivity Test




Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) CH₃OH B) H₂O A/B = 60/40, v/v
 Flow Rate : 1.0 mL / min Col. Temp.: 40 °C Detection : UV 254 nm
 Sample: 1. Uracil 2. Caffeine 3. Phenol 4; Butylbenzene
 5. Amylbenzene 6. o-Tertphenyl 7. Triphenylene

Acidic Compound Test




Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) ACN B) 0.1 % H₃PO₄ (H₂O) A/B = 75/25, v/v
 Flow Rate : 1.0 mL / min Col. Temp.: 40 °C
 Detection : UV 254 nm
 Sample: 1. Blue-FCF 2. Phenol 3. Salicylic Acid

Basic Compound Test 1 (Acidic mobile phase)




Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) ACN B) 0.1 % H₃PO₄ (H₂O) A/B = 75/25, v/v
 Flow Rate : 1.0 mL / min Col. Temp.: 40 °C
 Detection : UV 230 nm
 Sample: 1. Uracil 2. Dextromethorphan 3. Berberine

Basic Compound Test 2 (Neutral Mobile Phase)




Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) ACN B) 50 mM HCOONH₄ A/B = 70/30, v/v
 Flow Rate : 1.0 mL/min Col. Temp.: 40 °C
 Detection : UV 230 nm
 Sample: 1. Uracil 2. Dextromethorphan 3. Berberine

Separation of Cis-trans Test 1



Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) ACN B) 0.1 % H₃PO₄ (H₂O) A/B = 75/25, v/v
 Flow Rate : 1.0 mL/min Col. Temp.: 40 °C
 Detection : UV 210 nm
 Sample: 1. (S)-2-trans-4-trans-abscisic acid
 2. (S)-2-cis-4-trans-abscisic acid

Separation of Cis-trans Test 2



Column : 4.6 mm I.D × 150 mm, 5 μm
 Eluent: A) CH₃OH B) H₂O A/B = 30/70, v/v
 Flow Rate : 1.0 mL / min Col. Temp.: 40 °C
 Detection : UV 210 nm
 Sample: 1. Eugenol 2. cis-Isoeugenol 3. trans-Isoeugenol

Comparison of Performance 1/3

Selectivity Test


Acidic Compound

Basic Compound 1

Basic Compound 2

Separation of Cis-trans 1

Separation of Cis-trans 2

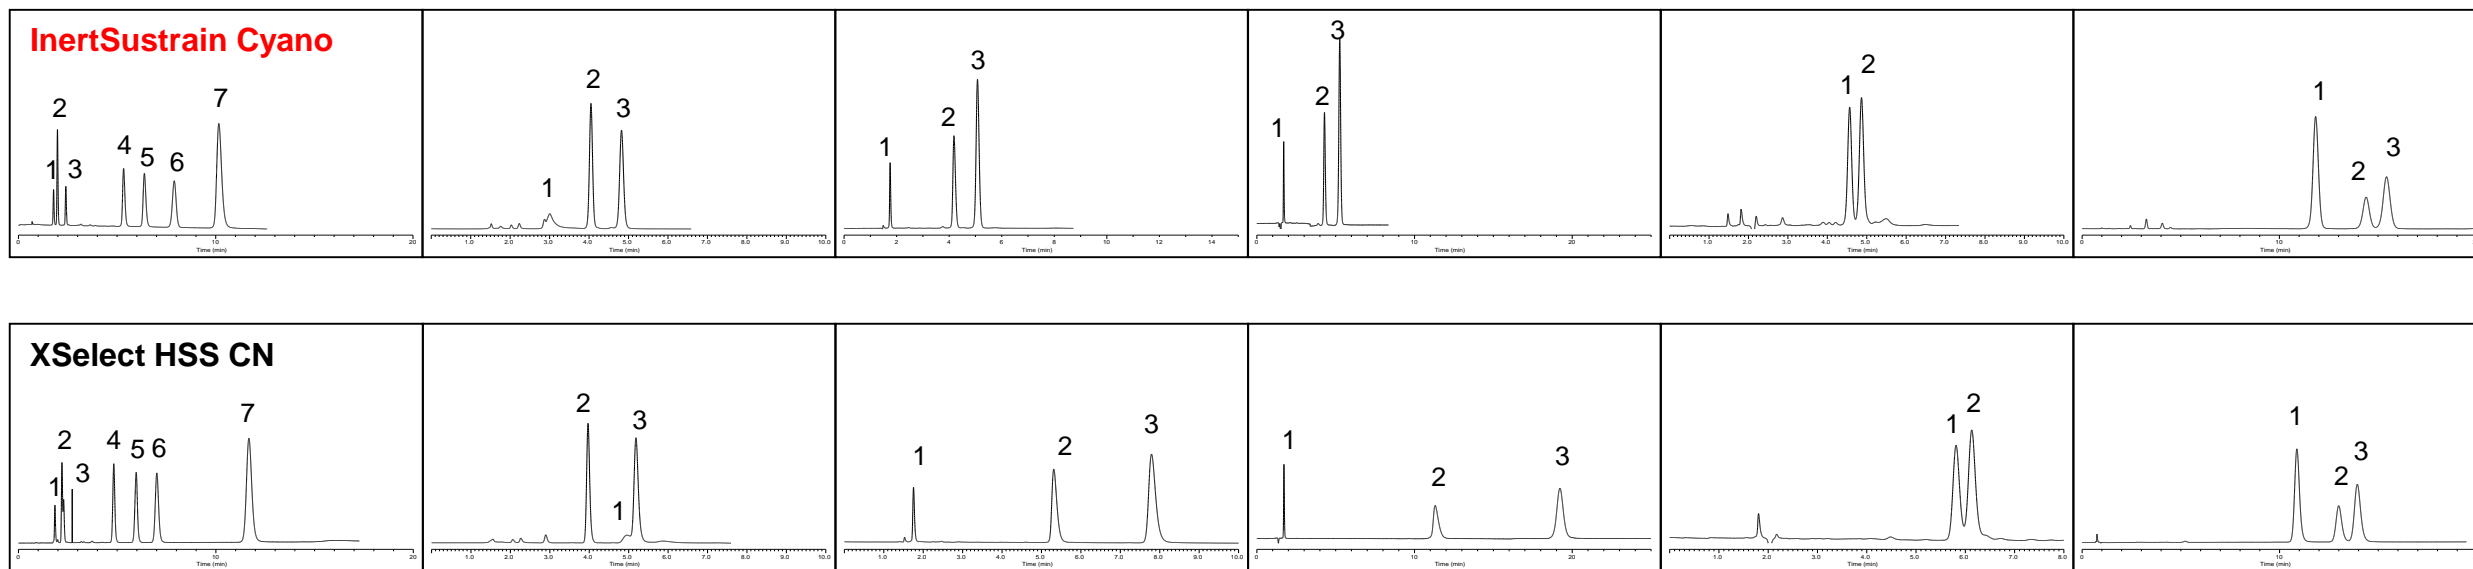

Comparison of Performance 2/3

Selectivity Test


Acidic Compound

Basic Compound 1

Basic Compound 2

Separation of Cis-trans 1

Separation of Cis-trans 2

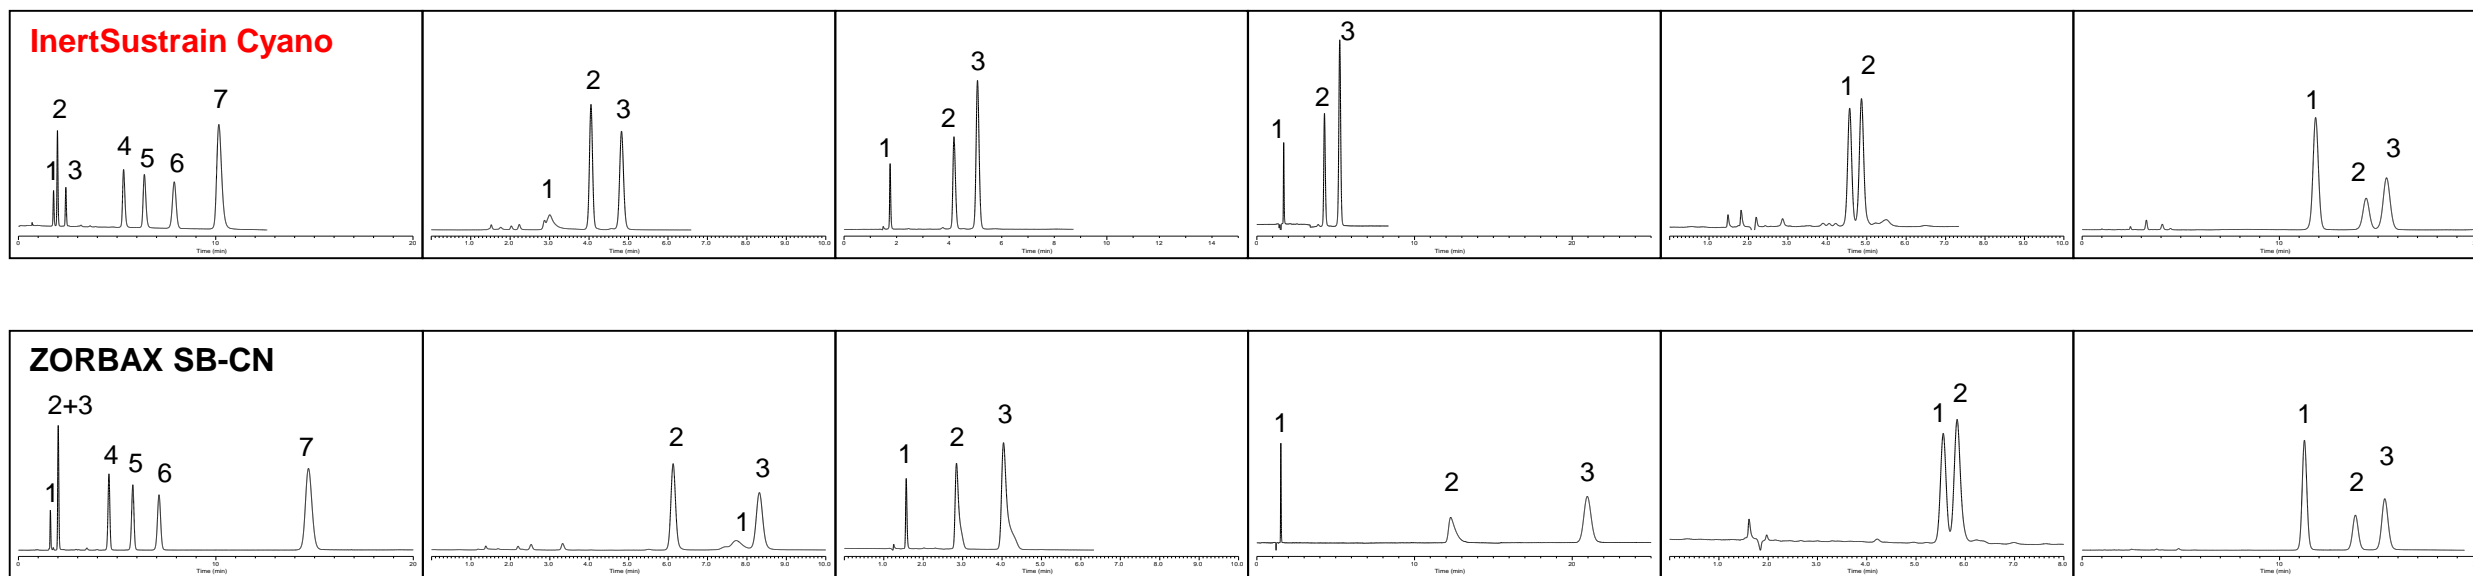

Comparison of Performance 3/3

Selectivity Test

Acidic Compound

Basic Compound 1

Basic Compound 2

Separation of Cis-trans 1

Separation of Cis-trans 2

